

Terlux® HD 2822
MABS

INEOS Styrolution

Terlux® HD 2822 is a standard-injection molding grade based on a MABS polymer. Terlux® HD 2822 offers a well balanced combination of stiffness and toughness and the high transparency well known in SAN molding compositions. Food contact statements are available on request.

Rheological properties	Value	Unit	Test Standard
ISO Data			
Melt volume-flow rate, MVR	2	cm ³ /10min	ISO 1133
Temperature	220	°C	-
Load	10	kg	-

Mechanical Properties	Value	Unit	Test Standard
ISO Data			
Tensile Modulus	2000	MPa	ISO 527
Yield stress	48	MPa	ISO 527
Yield strain	4	%	ISO 527
Nominal strain at break	12	%	ISO 527
Impact Strength (Charpy), +23°C	120	kJ/m ²	ISO 179/1eU
Impact Strength (Charpy), -30°C	80	kJ/m ²	ISO 179/1eU
Notched Impact Strength (Charpy), +23°C	5	kJ/m ²	ISO 179/1eA
Notched Impact Strength (Charpy), -30°C	2	kJ/m ²	ISO 179/1eA

Thermal Properties	Value	Unit	Test Standard
ISO Data			
Temp. of deflection under load (1.80 MPa)	90	°C	ISO 75-1/-2
Temp. of deflection under load (0.45 MPa)	94	°C	ISO 75-1/-2
Vicat softening temperature, 50°C/h 50N	93	°C	ISO 306

Other Properties	Value	Unit	Test Standard
ISO Data			
Water Absorption	0.7	%	Sim. to ISO 62
Humidity absorption	0.35	%	Sim. to ISO 62
Density	1080	kg/m ³	ISO 1183


Rheological calculation properties	Value	Unit	Test Standard
ISO Data			
Density of melt	960	kg/m ³	-
Thermal Conductivity of Melt	0.155	W/(m K)	-
Spec. heat capacity of melt	2060	J/(kg K)	-
Ejection temperature	90	°C	-

Test specimen production	Value	Unit	Test Standard
ISO Data			
Injection Molding, melt temperature	250	°C	ISO 294
Injection Molding, mold temperature	60	°C	ISO 294
Injection Molding, injection velocity	200	mm/s	ISO 294


Processing Recommendation Injection Molding	Value	Unit	Test Standard
Pre-drying - Temperature	70	°C	-
Pre-drying - Time	2	h	-
Melt temperature	230 - 260	°C	-
Mold temperature	50 - 80	°C	-

Diagrams


Viscosity-shear rate

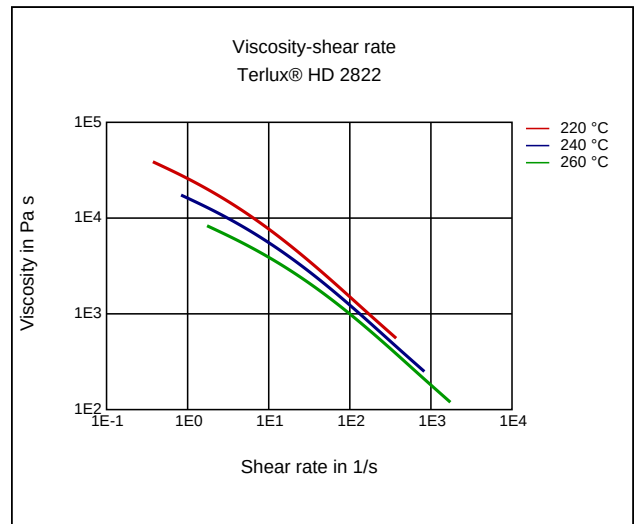


Shearstress-shear rate

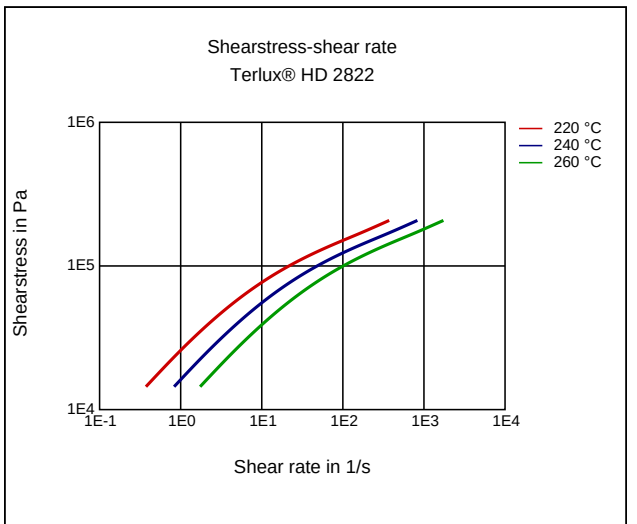


Stress-strain

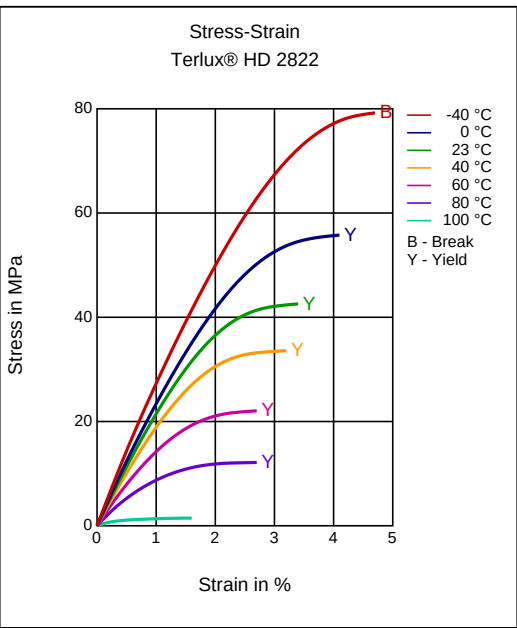


Secant modulus-strain

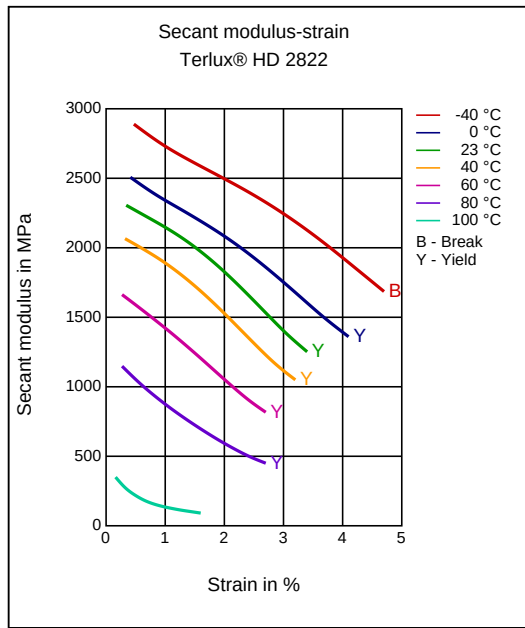


Stress-strain (isochronous) 23°C

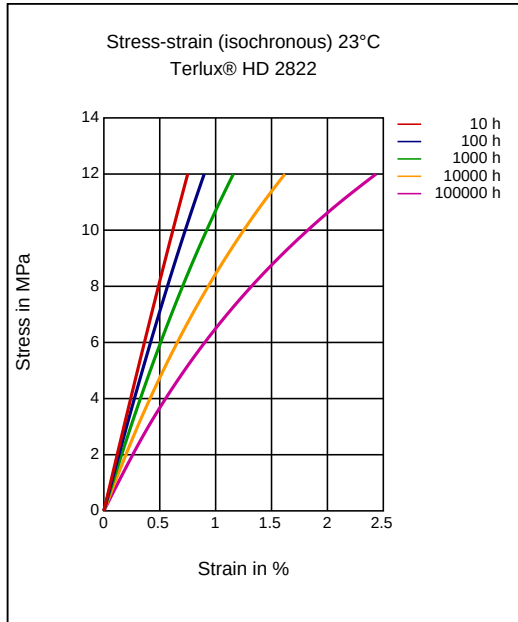


Creep modulus-time 23°C

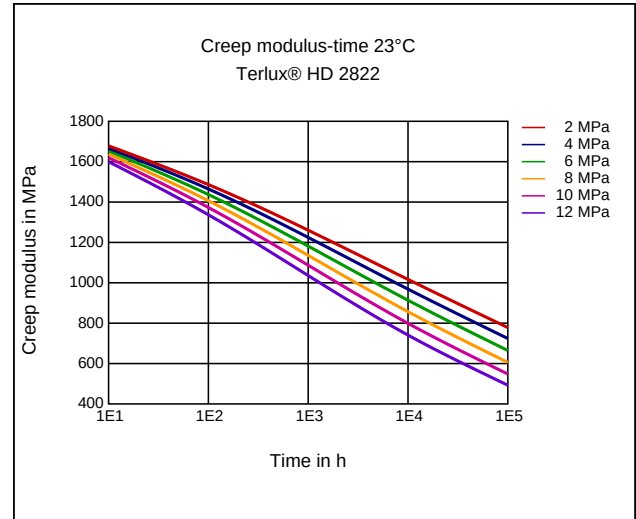


Stress-strain (isochronous) 40°C

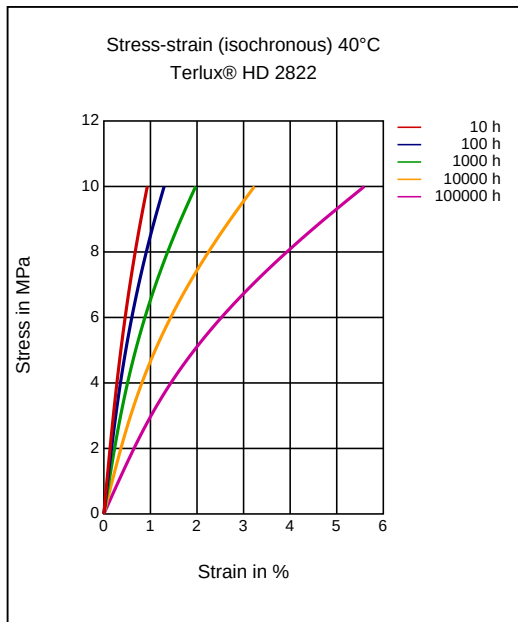


Creep modulus-time 40°C

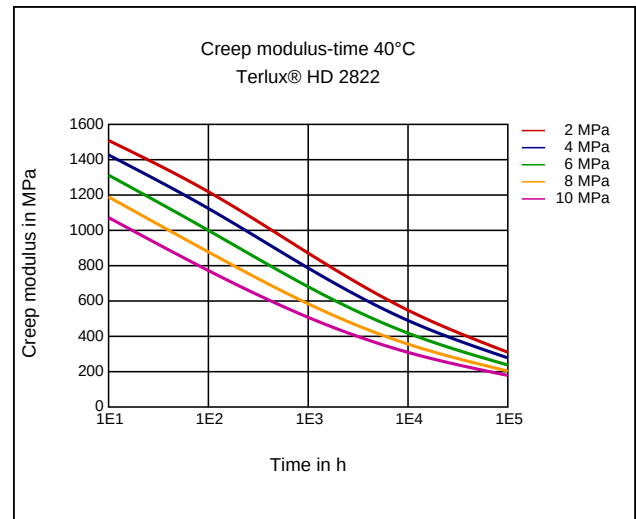


Stress-strain (isochronous) 60 °C

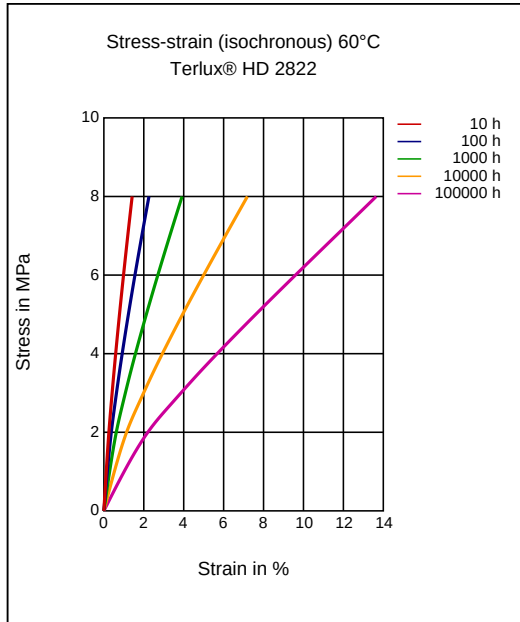

Creep modulus-time 60 °C

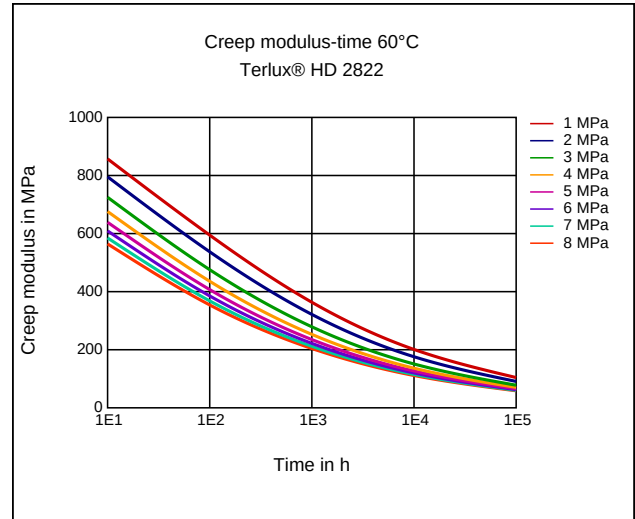

Specific volume-temperature (pvT)

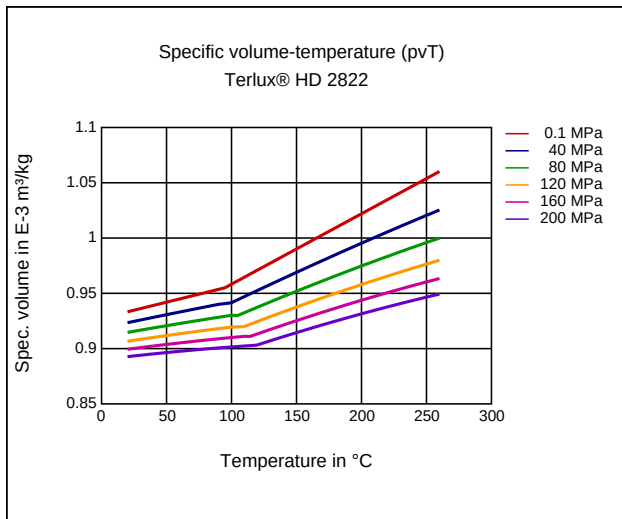

Characteristics

Processing

Injection Molding, Film Extrusion, Profile Extrusion, Sheet Extrusion, Blow Molding, Thermoforming

Delivery form

Pellets

Special Characteristics

Transparent, Sterilizable, Ethylene Oxide (EtO) Sterilization, Gamma irradiation sterilization

Injection Molding

PREPROCESSING

Chemical Resistance

Radiation Resistance

Certifications

Medical, Biocompatibility ISO 10993, US Pharmacopeia Class VI Approved, Drug Master File, Long term supply assurance, Food approval, Food approval 10/2011, Food Contact (FDA)

Applications

Medical

Pre-drying, Temperature: 70 °C

Pre-drying, Time: 2 h

PROCESSING

Melt temperature, range: 230 - 260 °C

Melt temperature, recommended: 245 °C

Mold temperature, range: 50 - 80 °C

Mold temperature, recommended: 65 °C

Disclaimer

Liability Exclusion

These guide values are measured and provided by the product manufacturer and have been determined on standardised test specimens and can be affected by pigmentation, mould design and processing conditions. M-Base has taken the guide values from the producer's original Technical Data Sheet. **ALBIS AND M-BASE ARE THEREFORE NOT RESPONSIBLE FOR THE ACCURACY OF THE GUIDE VALUES AND CANNOT GIVE ANY WARRANTY WITH REGARD TO THEIR CORRECTNESS.**

Any information given on the chemical and physical characteristics of our products, including, without limitation, technical advice on applications, whether verbally, in writing or by testing the product, is given to the best of our knowledge and in good faith and does not exempt the buyer from carrying out their own investigations and tests in order to ascertain the product's specific suitability for the purpose intended.

The buyer is solely responsible for confirming the suitability of the product for a particular application, its utilization and processing and must observe any applicable laws and government regulations. **NO EXPRESS OR IMPLIED RECOMMENDATION OR WARRANTY IS GIVEN WITH REGARD TO THE SUITABILITY OF THE PRODUCT FOR A PARTICULAR APPLICATION, SUCH AS, BUT NOT LIMITED TO, SAFETY-CRITICAL COMPONENTS OR SYSTEMS.**

Healthcare uses: the supply of any product by ALBIS for any medical, pharmaceutical or diagnostic application is conditional to an assessment by ALBIS in terms of compliance with ALBIS' internal risk management policy – even for products which are in general designated for use in Healthcare applications.

Important: irrespective of product type or designation, ALBIS does not recommend or support the use of any products it supplies which fall into the following medical, pharmaceutical or diagnostic application categories:

- risk class III applications according to EU directive 93/42/EEC
- any bodily implant application for greater than 30 days
- any critical component in any medical device that supports or sustains human life.

At all times, our standard terms and conditions of sale apply.